

# **N-Ethyl-U-47700**

Sample Type: Seized Material

CI

Latest Revision: March 24, 2020

Date of Report: March 24, 2020

### 1. GENERAL INFORMATION

**IUPAC Name:** 3,4-dichloro-N-[2-(dimethylamino)cyclohexyl]-N-ethyl-benzamide

**InChI String:** InChI=1S/C17H24Cl2N2O/c1-4-21(16-8-6-5-7-15(16)20(2)3)17(22)12-9-

10-13(18)14(19)11-12/h9-11,15-16H,4-8H2,1-3H3

**CFR:** Not Scheduled (03/2020)

CAS# Not Available

**Synonyms:** Ethyl U-47700

**Source:** Franklin County Coroner's Office (Columbus, OH)

**Appearance:** White Solid Material

#### 2. CHEMICAL DATA

Analyte	Chemical	Molecular	Molecular	Exact Mass
	Formula	Weight	Ion [M <sup>+</sup> ]	[M+H] <sup>+</sup>
N-Ethyl-U-47700	$C_{17}H_{24}Cl_2N_2O$	343.3	342	343.1338

*Important Note*: All identifications were made based on evaluation of analytical data (e.g. GC-MS, LC-QTOF-MS) in comparison to analysis of acquired reference material.

**Report Prepared By:** Alex J. Krotulski, PhD; Daniel Baker, MS, F-ABFT; Nancy E. Kelly; and Barry K. Logan, PhD, F-ABFT

#### 3. BRIEF DESCRIPTION

*N*-Ethyl-U-47700 is classified as a novel opioid. Novel opioids have been reported to cause opioid-like effects similar to heroin and fentanyl. Novel opioids in the trans-N-[2-(methylamino)cyclohexyl]-benzamide class (e.g. U-47700) and similar classes (e.g. U-49900) have caused adverse events, including deaths, as described in the literature. U-47700 is a Schedule I substance in the United States; no other U-series analogues are explicitly scheduled.

#### 4. ADDITIONAL RESOURCES

https://www.caymanchem.com/product/24899/

## 5. QUALITATIVE DATA

#### **5.1 GAS CHROMATOGRAPHY MASS SPECTROMETRY (GC-MS)**

**Testing Performed At:** The Center for Forensic Science Research and Education at the

Fredric Rieders Family Foundation (Willow Grove, PA)

**Sample Preparation:** Drug material diluted in methanol

**Instrument:** Agilent 5975 Series GC/MSD System

**Column:** Agilent J&W DB-1 (12 m x 200 μm x 0.33 μm)

Carrier Gas: Helium (Flow: 1.46 mL/min)

**Temperatures:** Injection Port: 265 °C

Transfer Line: 300 °C

MS Source: 230 °C

MS Quad: 150 °C

Oven Program: 50 °C for 0 min, 30 °C/min to 340 °C for 2.3 min

**Injection Parameters:** Injection Type: Splitless

Injection Volume: 1 µL

**MS Parameters:** Mass Scan Range: 40-550 m/z

Threshold: 250

**Retention Time:** 7.08 min

**Standard Comparison:** Reference material for *N*-Ethyl-U-47700 (Batch: 0581748-1) was


purchased from Cayman Chemical (Ann Arbor, MI, USA).

Analysis of this standard resulted in positive identification of the analyte in the exhibit as *N*-Ethyl-U-47700, based on retention time

(7.04 min) and mass spectral data.


(https://www.caymanchem.com/product/24899/).

# Chromatogram: N-Ethyl-U-47700

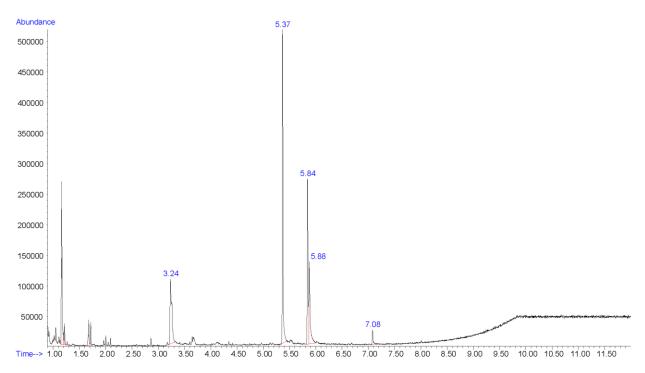

Additional peaks in chromatogram: internal standard (3.24 min), lidocaine (5.37 min), internal standard (5.84 min), and 3,4-Difluoro-U-47700 (5.88 min)

EI (70 eV) Mass Spectrum: N-Ethyl-U-47700

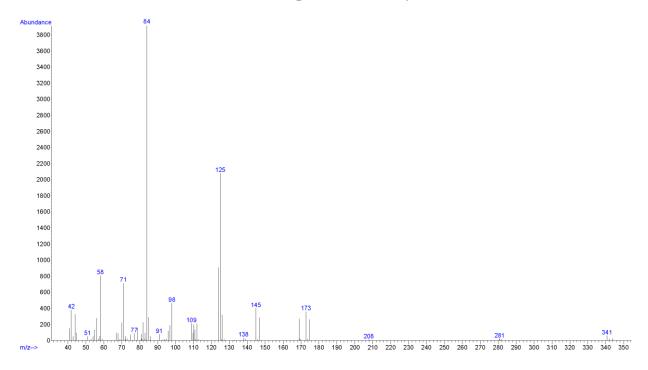

# **5.2 LIQUID CHROMATOGRAPHY QUADRUPOLE TIME-OF-FLIGHT MASS SPECTROMETRY (LC-QTOF-MS)**

**Testing Performed At:** The Center for Forensic Science Research and Education at the

Fredric Rieders Family Foundation (Willow Grove, PA)

**Sample Preparation:** 1:100 dilution in mobile phase of GC-MS methanolic dilution

**Instrument:** Sciex TripleTOF® 5600+, Shimadzu Nexera XR UHPLC

Column: Phenomenex® Kinetex C18 (50 mm x 3.0 mm, 2.6 μm)

**Mobile Phase:** A: Ammonium formate (10 mM, pH 3.0)

B: Methanol/acetonitrile (50:50)

Flow rate: 0.4 mL/min

**Gradient:** Initial: 95A:5B; 5A:95B over 13 min; 95A:5B at 15.5 min

**Temperatures:** Autosampler: 15 °C

Column Oven: 30 °C

Source Heater: 600 °C

**Injection Parameters:** Injection Volume: 10 µL

**QTOF Parameters:** TOF MS Scan Range: 100-510 Da

Precursor Isolation: SWATH® acquisition (27 windows)

Fragmentation: Collison Energy Spread (35±15 eV)

MS/MS Scan Range: 50-510 Da

**Retention Time:** 6.68 min

**Standard Comparison:** Reference material for *N*-Ethyl-U-47700 (Batch: 0581748-1) was

purchased from Cayman Chemical (Ann Arbor, MI, USA).


Analysis of this standard resulted in positive identification of the

analyte in the exhibit as N-Ethyl-U-47700, based on retention time

(6.70 min) and mass spectral data.


(https://www.caymanchem.com/product/24899/).

## Chromatogram: N-Ethyl-U-47700

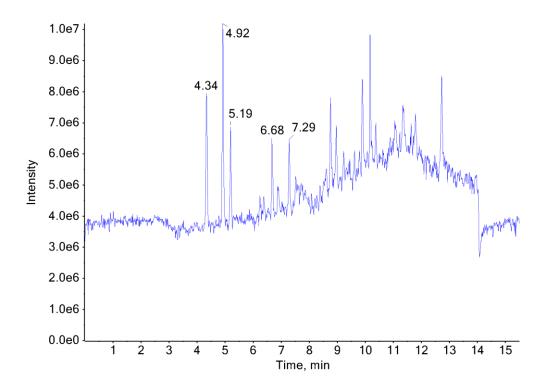


Additional peaks in chromatogram: lidocaine (4.34 min), internal standard (4.92 min), 3,4-Difluoro-U-47700 (5.19 min), and internal standard (7.29 min)

TOF MS Spectrum: N-Ethyl-U-47700

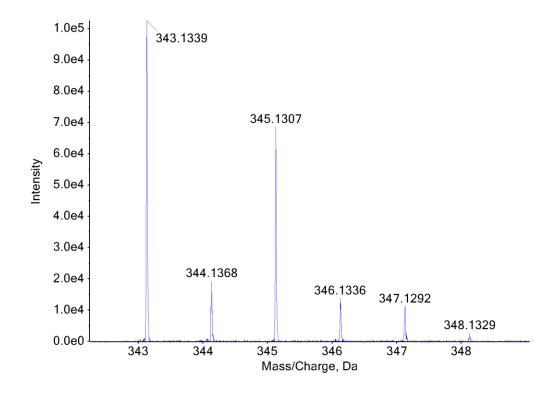

MS/MS Spectrum: N-Ethyl-U-47700

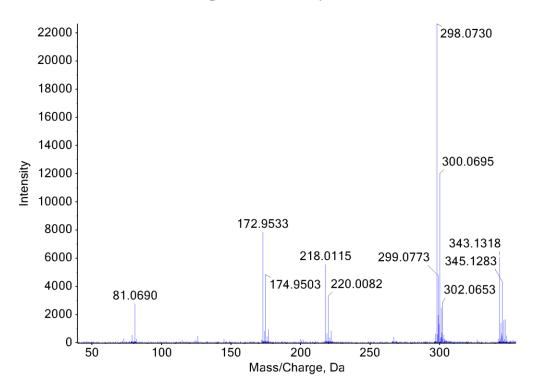

Page **6** of **6**